SIEMENS

MAMMOMAT 300/3000

SP

Service

Installation Instructions

AEC Detector mask

Kit; 62 98 728 X041E

© Siemens-Elema AB 1997
The reproduction, transmission or use of this document or its contents is not permitted without express written authority. Offenders will be liable for damages. All rights, including rights created by patent grant or registration of a utility model or design, are reserved.

Register 5
Print No.: SPB7-120.031.12.01.02
Replaces:

English
Doc. Gen. Date: 04.97
64 59 502

General

Purpose

This is an instruction of how to mount an AEC Detector mask for small breast at the object table

Time required

1 h for 1 person

Contents of the kit

The kit 62 98 728 X041E contains of following parts:

Pos.	Amount	Name
A	1	Detector mask
B	1	Holder for Detector mask
C	1	Label
-	1	Installation Instructions (english), 64 59 502
D	1	Supplement to Operating Instructions (english), 64 59 486 (text stripes to place in the Operating Instructions)
E	1	
F	1	

Procedure

Kit installation

Placing the detector mask holder

1 Remove the protective paper from the tape straps on the detector mask holder.

2 Place the holder **B** at the table locking device and press to get it fixed by the tape.

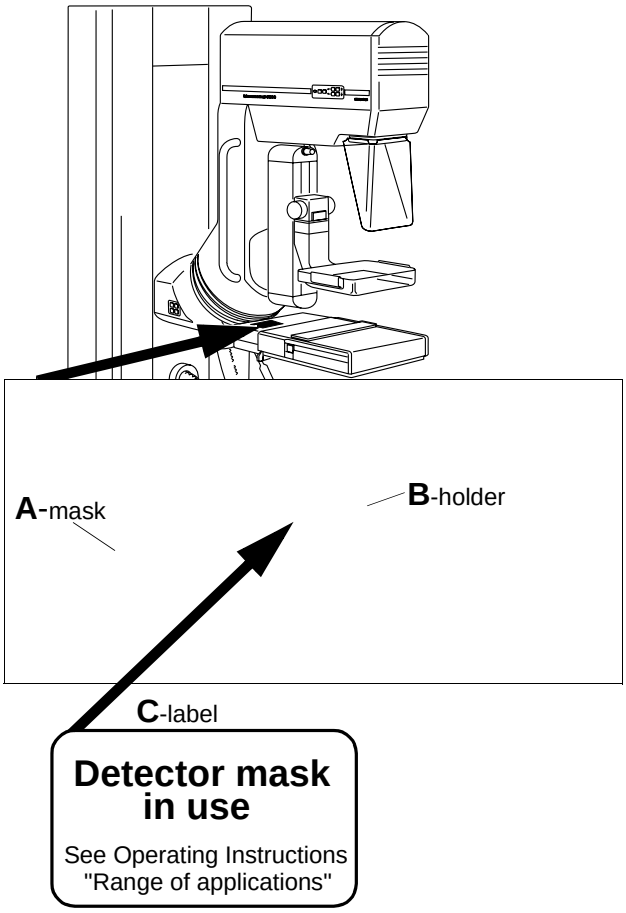

Place the label on the object table

3 Place the self-adhesives label **C** on the object table as shown in figure beside.

Place the mask into the holder

4 Place the AEC Detector mask **A** into its holder with its magnet facing the cover plate.

Place supplemented text stripes in the Operating Instructions

5 Cut out and place the supplemented text stripes from the self-adhesives sheet into Operating Instructions as shown below.



This page intentionally left blank.